



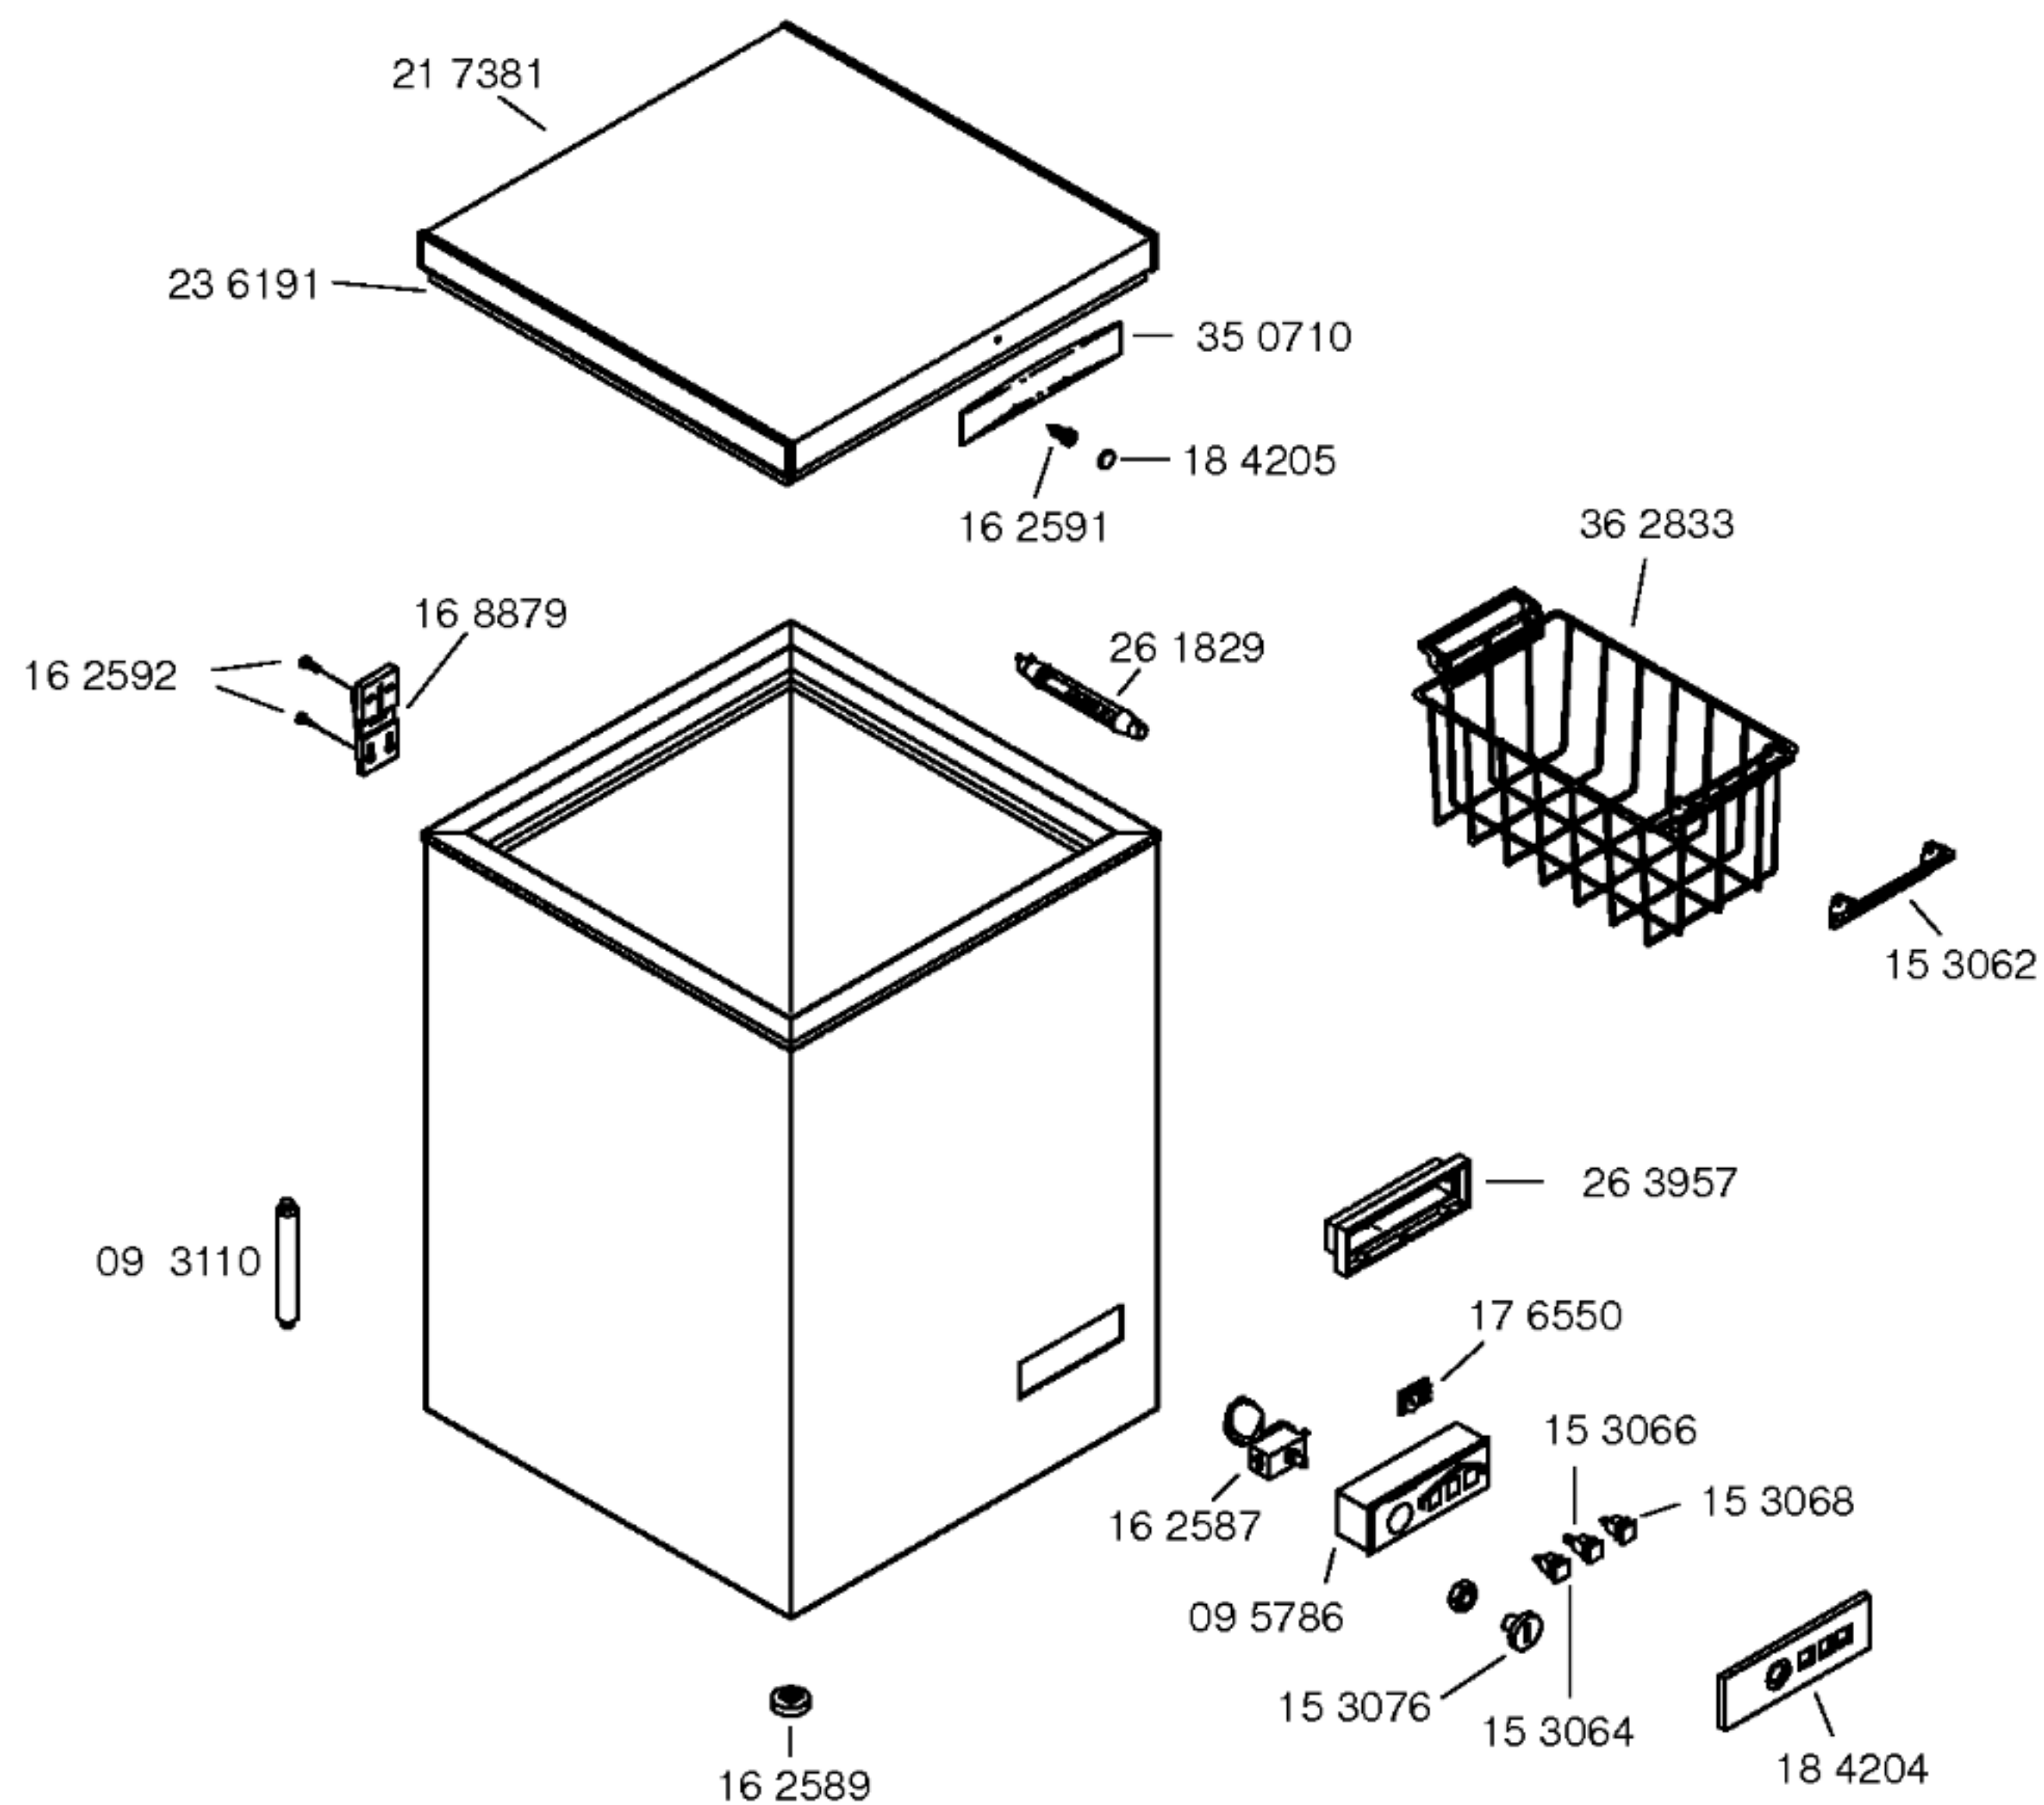

Mat. – Nr. – Konstante
3740
Gebrauchsanweisung
52 9302
(D,GB,TR)

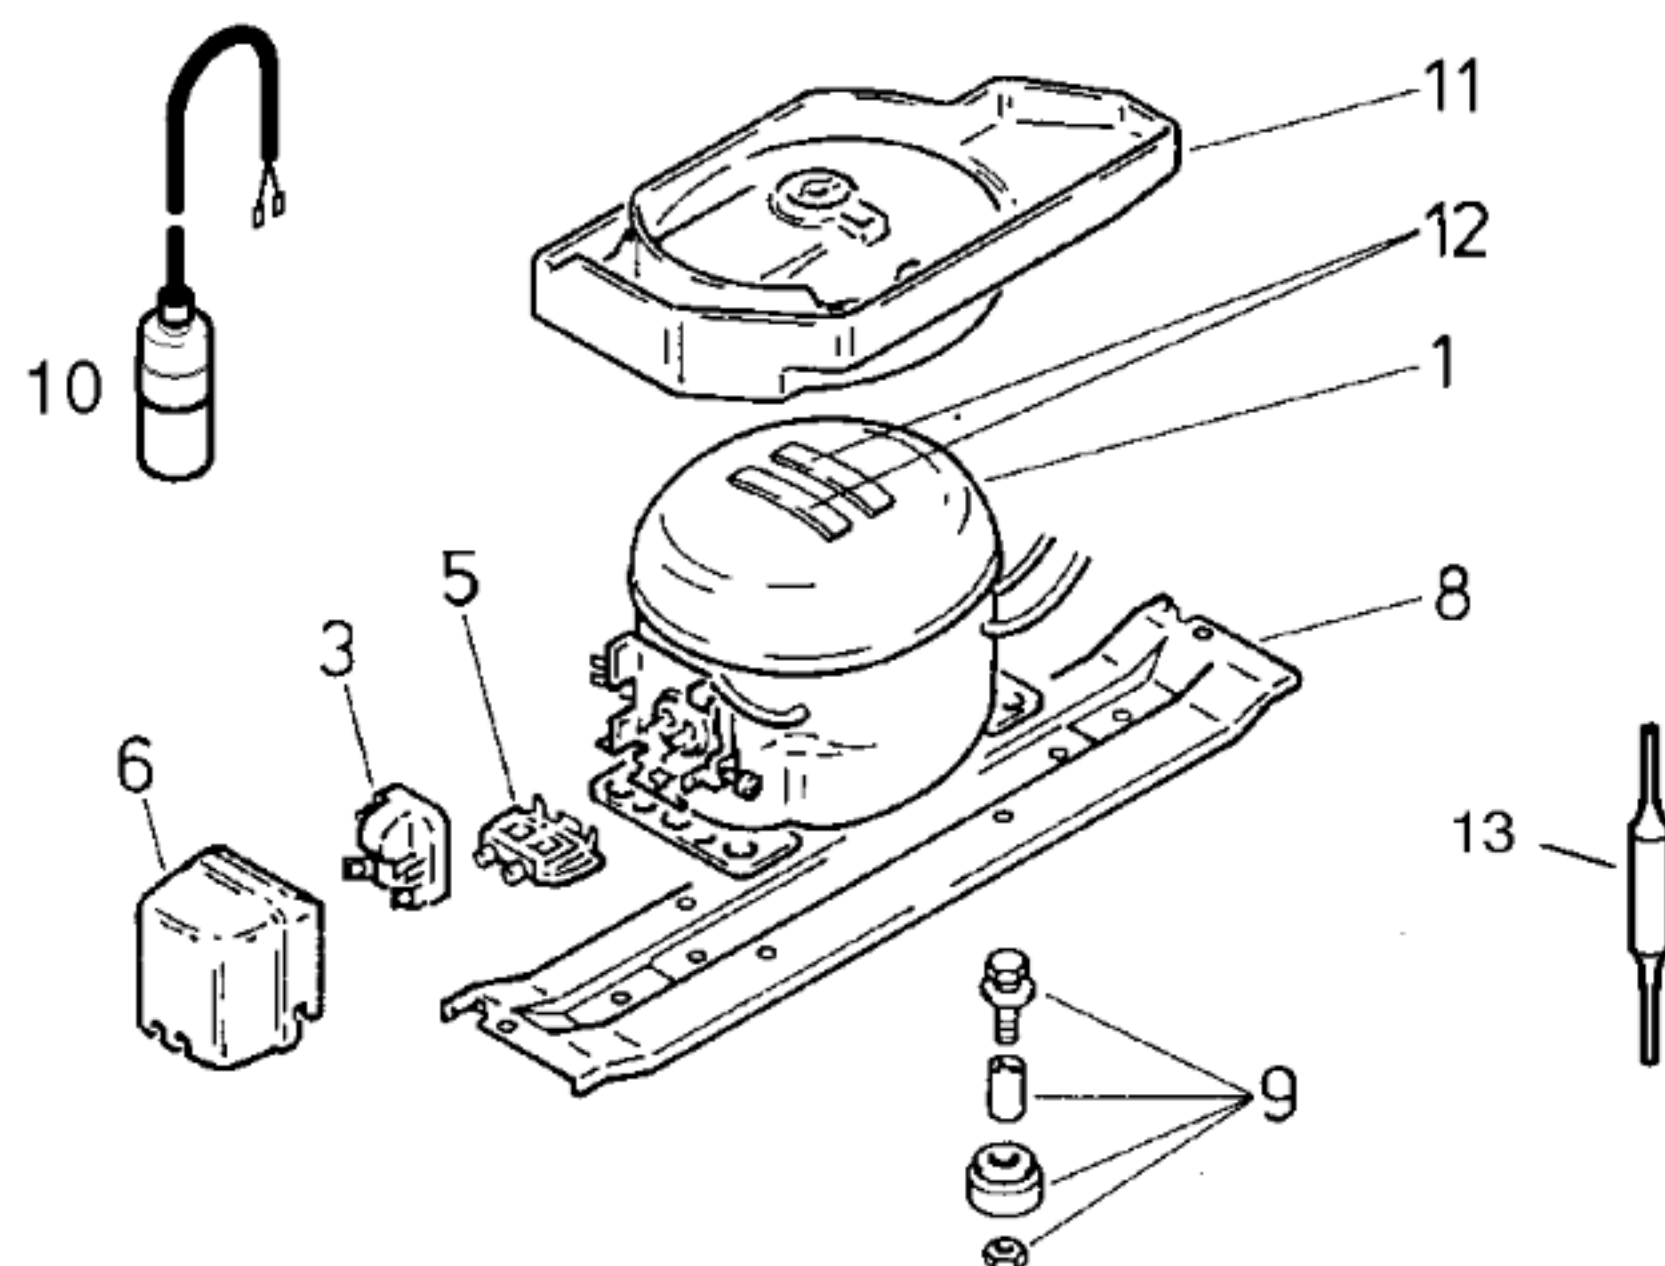

	V01	V02	V03
Pos.	Zanussi HLY 55AA	Matsushita SD65E	Danfoss TLES6KK2
1	14 2186	141981	14 1904
2			
3	18 4206	15 3306	15 1055
4			
5	15 3080	15 3865	15 0760
6	15 3079	15 3303	15 1072
7			
8			
9	16 7400	16 7400	16 7400
10			
11			
12			
13			

TECHNISCHE DATEN / TECHNICAL DATA / DONNEES TECHNIQUES			
Verdichter/Compressor/Compresseur	Zanussi HLY 55AA	Matsushita SD65E	Danfoss TLES6KK2
Typ/Type			
Förderleistung/Delivery/Débit	l/h		
Anlaufstrom/Starting current/Cour de démarrage	A		
Widerstand/Resistance/Résistance Ha/main/prin	Ω		
Hi/aux	Ω		
Temp.-Regler/Thermostat			
Typ/Type			
Regelstellung/Position			
Schaltwerte/Switching values	"warm"		
Valeurs de commutation	"kalt"		
	"alarm"		
Füllmenge/Fill.quantity/Charge	R600a		
Anschlußwert/Conn.load/Puiss. connectée	W		
Heizung/Heater/Chauffage			
Widerstand/Resistance/Résistance	Ω		
Leistung/Power/Puissance	W		
Ventilator/Blower/Ventilateur			
Widerstand/Resistance/Résistance	Ω		
Temp.-Regler/Thermostat			
Magnetventil/Magnetic valve/Electrovanne			
Widerstand/Resistance/Résistance	Ω		
Spannung/Voltage/Tension	V		